


**Tra cứu phân loại của FDA - Mỹ bằng cách nhấp chuột vào đường link sau:**

<https://www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfRL/rl.cfm?lid=449701&lpcd=JJM>

Thông tin phân loại hiển thị như sau:

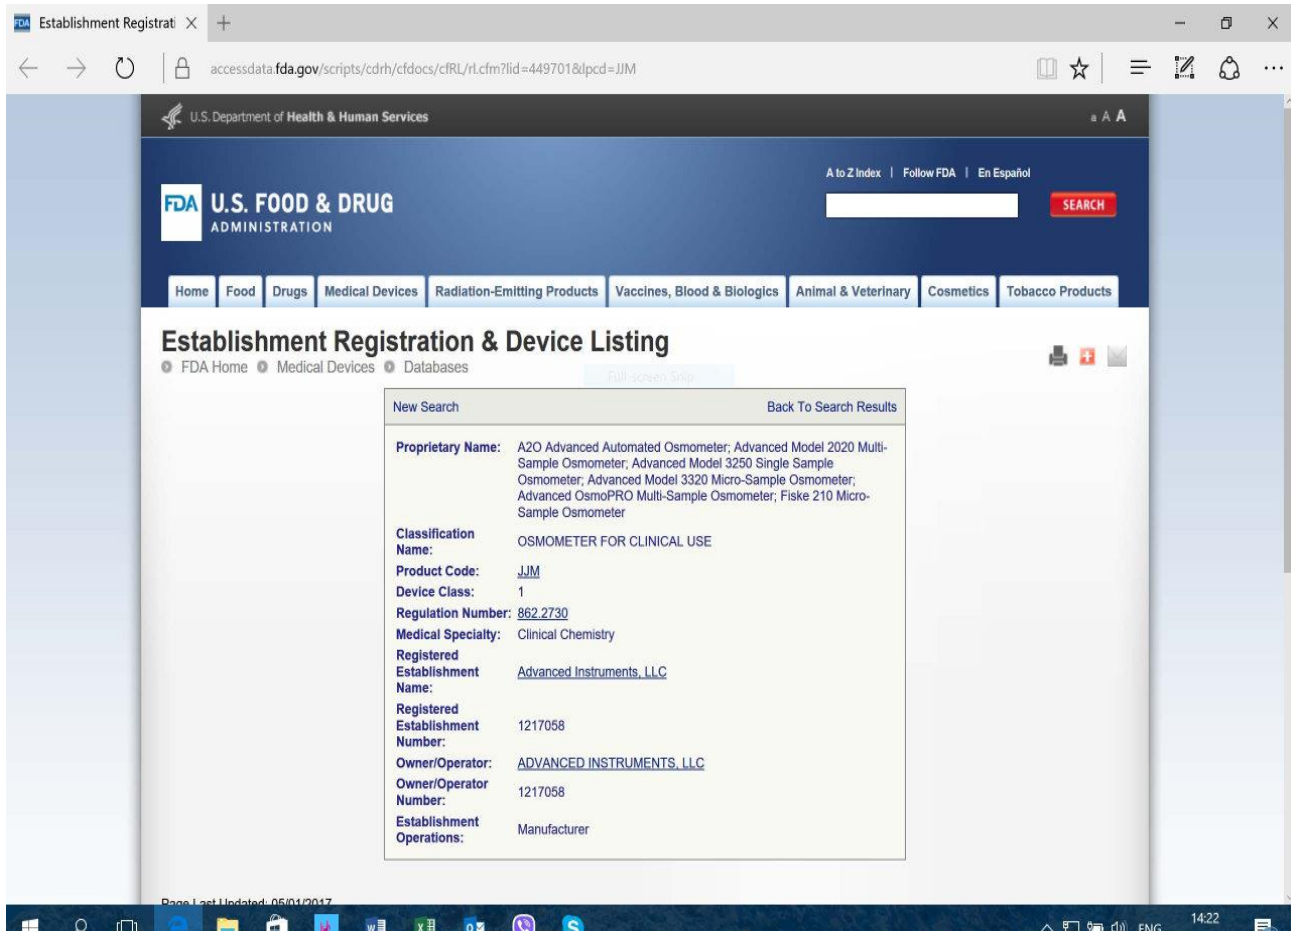

The screenshot shows the FDA's Establishment Registration & Device Listing page. The page header includes the U.S. Department of Health & Human Services logo and the FDA logo. The main content area displays the following information:

New Search		Back To Search Results
<b>Proprietary Name:</b>	A20 Advanced Automated Osmometer; Advanced Model 2020 Multi-Sample Osmometer, Advanced Model 3250 Single Sample Osmometer, Advanced Model 3320 Micro-Sample Osmometer; Advanced OsmoPRO Multi-Sample Osmometer; Fiske 210 Micro-Sample Osmometer	
<b>Classification Name:</b>	OSMOMETER FOR CLINICAL USE	
<b>Product Code:</b>	<a href="#">JJM</a>	
<b>Device Class:</b>	1	
<b>Regulation Number:</b>	<a href="#">862.2730</a>	
<b>Medical Specialty:</b>	Clinical Chemistry	
<b>Registered Establishment Name:</b>	<a href="#">Advanced Instruments, LLC</a>	
<b>Registered Establishment Number:</b>	1217058	
<b>Owner/Operator:</b>	<a href="#">ADVANCED INSTRUMENTS, LLC</a>	
<b>Owner/Operator Number:</b>	1217058	
<b>Establishment Operations:</b>	Manufacturer	

**Người đại diện hợp pháp của cơ sở**

